


## TABLE OF CONTENTS

	<b>Page</b>
ACKNOWLEDGEMENTS	iii
ABSTRACT (THAI)	iv
ABSTRACT (ENGLISH)	v
LIST OF TABLES	ix
LIST OF FIGURES	x
CHAPTER 1 INTRODUCTION	1
CHAPTER 2 SYSTEMATIC LITERATURE REVIEW: MAXILLARY MOLAR DISTALIZATION WITH OR WITHOUT TEMPORARY ANCHORAGE DEVICES	
1.1 Introduction	4
1.2 Materials and methods	5
1.3 Results	6
1.4 Discussion	17
1.5 Conclusions	19
CHAPTER 3 ANATOMY OF THE PALATE AND INSERTION TORQUE OF MINISCREW IMPLANT PLACEMENT	20
CHAPTER 4 ASSESSMENT OF MAXIMUM INSERTION TORQUE DURING MINISCREW IMPLANT PLACEMENT IN DIFFERENT AREAS OF THE PALATE	
2.1 Introduction	28
2.2 Materials and methods	29

ลิขสิทธิ์งานวิจัยนี้สงวนไว้  
Copyright © by Chiang Mai University  
All rights reserved

2.3 Results	34
2.4 Discussion	37
2.5 Conclusions	41
BIBLIOGRAPHY	43
APPENDIX	52
CURRICULUM VITAE	57

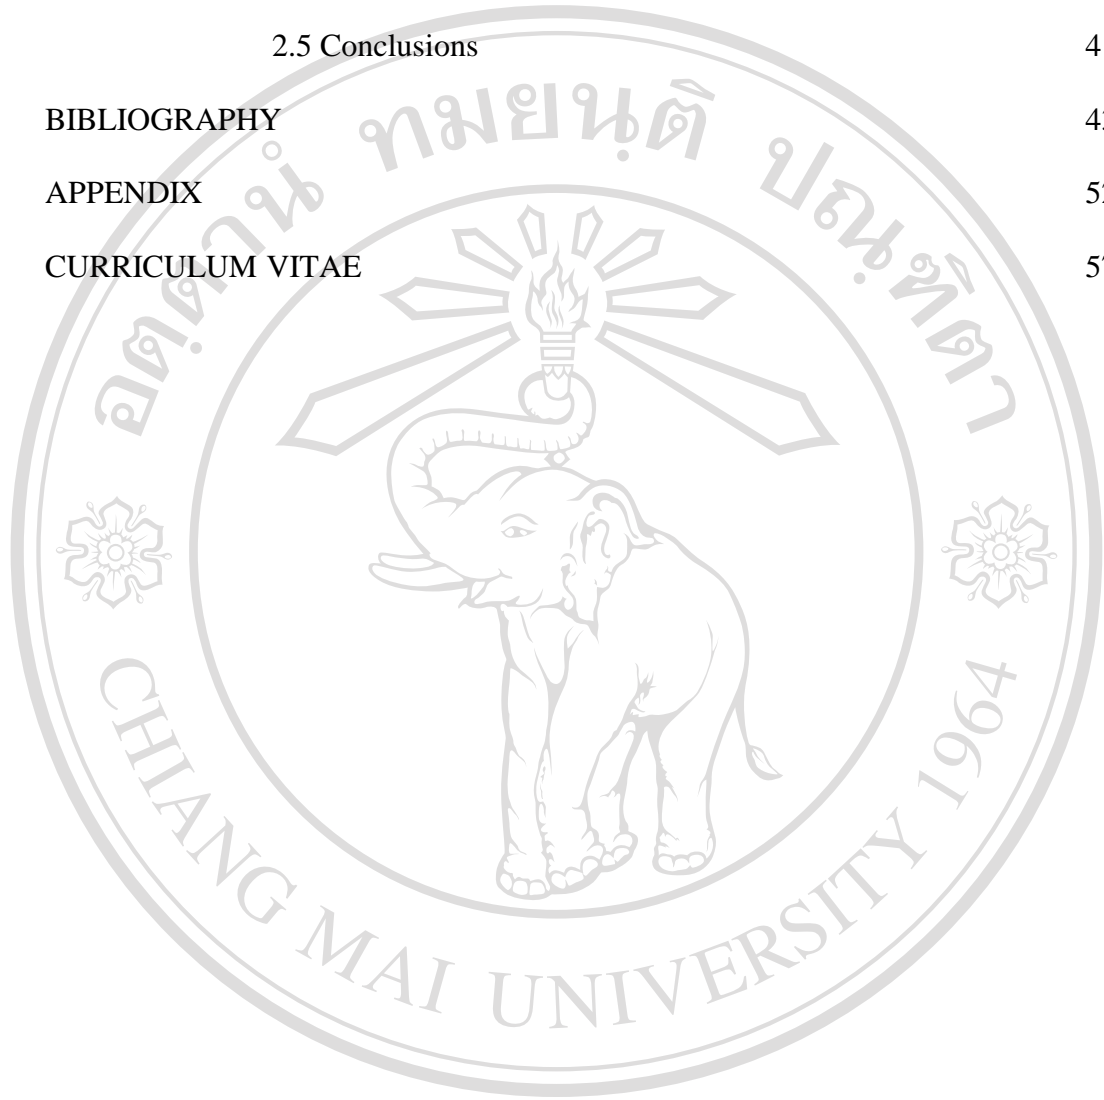

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่  
Copyright© by Chiang Mai University  
All rights reserved


## LIST OF TABLES

<b>Table</b>		<b>Page</b>
2.1	Details of conventional distalizing device studies included for data analysis.	7
2.2	Details of miniscrew implant supported distalizing device studies included for data analysis.	9
2.3	Heterogeneity assessment of amount of molar distalization in conventional distalizing device.	10
2.4	Heterogeneity assessment of amount of molar distalization in miniscrew implant supported distalizing device.	10
2.5	Rate of molar distalization in conventional distalizing devices.	13
2.6	Rate of molar distalization in distalization with miniscrew implant supported distalizing devices.	14
2.7	Force magnitudes in conventional distalizing devices.	16
2.8	Force magnitudes in miniscrew implant supported distalizing devices.	17
4.1	Maximum insertion torque value (Ncm) at each measurement site.	34
4.2	Maximum insertion torque value (Ncm) between parasagittal and midpalatal.	34
4.3	Maximum insertion torque value (Ncm) between the anterior, middle and posterior sites.	35

## LIST OF FIGURES

Figure		Page
2.1	Forest plot for the mean amount of molar distalization for conventional distalizing devices.	12
2.2	Forest plot for the mean amount of molar distalization for miniscrew implant supported distalizing devices.	12
2.3	Forest plot for the mean amount of molar distal tipping in conventional distalizing devices.	15
2.4	Forest plot for the mean amount of molar distal tipping in miniscrew implant supported distalizing devices.	15
3.1	Anatomy of the palate.	22
3.2	Foramina of the palate, blood vessels and nerves.	22
3.3	Midpalatal suture and parasagittal regions.	23
3.4	Ossification of the midpalatal palatal suture in transversal section through the midpalatal region.	24
3.5	Bone thickness of the palate.	24
3.6	Load and deflection curve of Ti-6Al-4V titanium alloy.	26
3.7	Insertion torque for miniscrew implant until fracture.	26
4.1A	Self-drilling titanium miniscrew implants used in the present study.	30
4.1B	Hard palate of cadaver.	30
4.2	Palatal bone, a total on nine miniscrews were marked by a template.	31

4.3	Miniscrew implant placement sites.	32
4.4A	Imada torque wrench (DIS-RL, Imada Inc., Northbrook, USA).	33
4.4B	Jacobs chuck of the torque wrench for applied to the miniscrew.	33
4.5	Box plot graph of maximum insertion torque value (Ncm) of parasagittal and midpalatal suture regions.	35
4.6	Box plot graph of maximum insertion torque value (Ncm) between the anterior, middle and posterior sites.	36

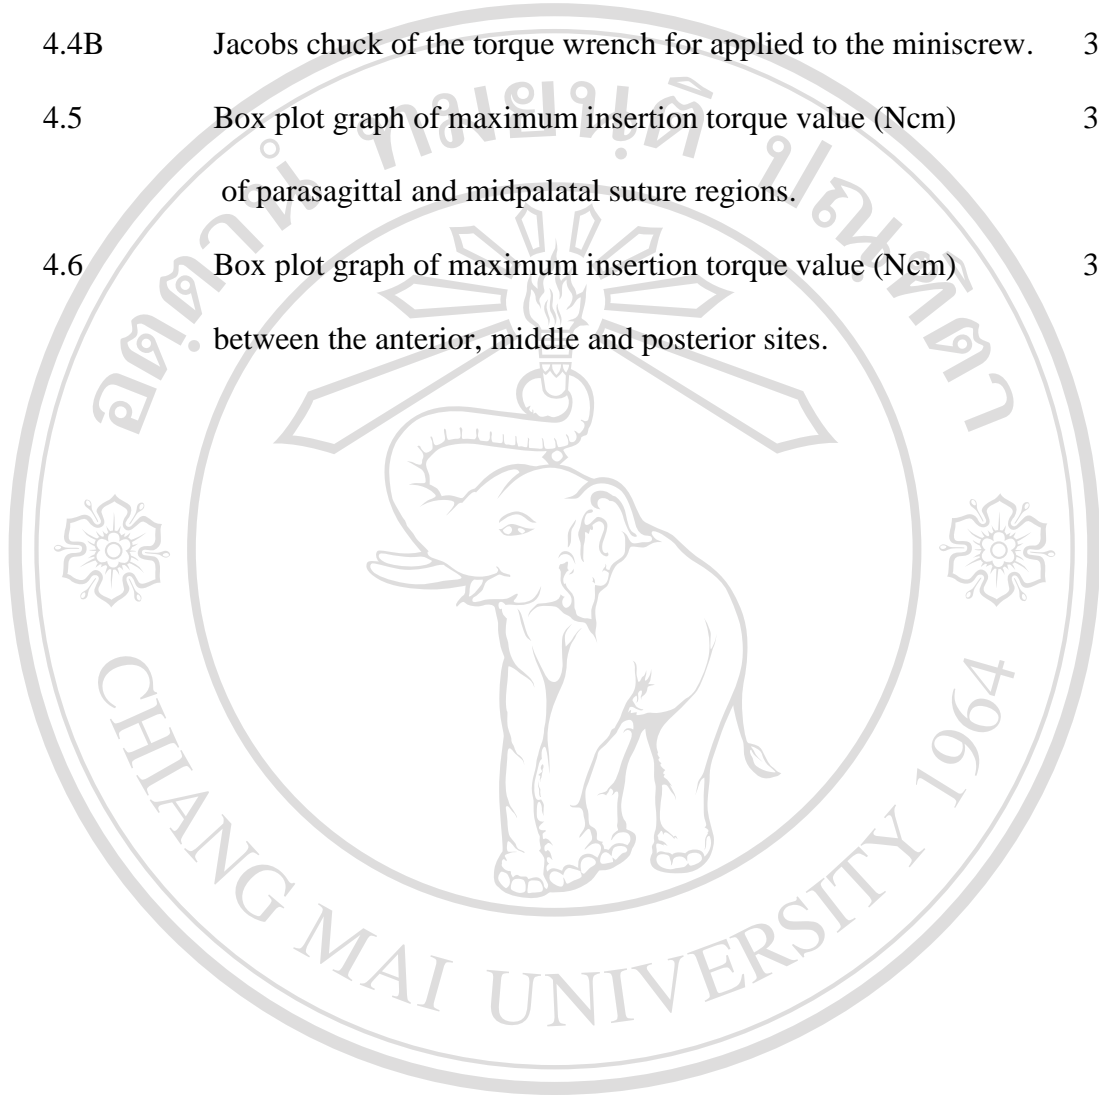

ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่  
Copyright© by Chiang Mai University  
All rights reserved



ลิขสิทธิ์มหาวิทยาลัยเชียงใหม่

Copyright© by Chiang Mai University

All rights reserved